



Date: 2011-08-04

File number: AP-AG-11-0028

MODIFICATION ACCEPTANCE LETTER (MAL) FOR Approved Meters and Devices

Type of Device

Electronic Volume Transponder
(Encoder/Receiver/Transmitter)

Purpose

The purpose of this letter is to convey details of modifications to meters which have previously received approval of type recognition from Measurement Canada. These modifications have been evaluated by the Approval Services Laboratory in accordance with national requirements and shall be considered to be included within the scope of the originally issued Notices of Approval specified in this document and any subsequent revisions to these Notices of Approval.

Scope

The modifications described in this letter affect meters identified in the following Notice (s) of Approval:

Approval Numbers

AG-0546

Applicant

Itron Canada Inc.
6507C Mississauga Road
Mississauga, Ontario
Canada, L5N 1A6

Description of Modifications

The Itron Encoder/Receiver/Transmitter approved under AG-0546 can be used with the following host meter models:

| Device Manufacturer | Model | Itron Part Number |
|--|---|--------------------------------|
| Actaris / Schlumberger | 675A, M675A, 800A, M800A, 1000A, M1000A | ERG-5000-007 |
| Elster American Meter / American Meter Company | 35B, 80B, 250B, 500B, AL800, ALM800, AL1000, ALM1000 | ERG-5000-007 |
| Elster American Meter / American Meter Company | AL1400, AL2300 | ERG-5003-007 and ERG-5003-007P |
| Sensus Metering Systems | RCM-750 | ERG-5003-008 and ERG-5003-008P |

The Actaris meters require adapter P/N 80005901 available from Actaris.

Original signed by:

Randy Byrtus, CET
Manager, Gas Measurement



Date: 2011-08-04

Dossier: AP-AG-11-0028

LETTRE D'ACCEPTATION DE MODIFICATION (LAM) pour Compteurs et appareils approuvés

Type d'appareil

Transpondeur électronique de volume
(encodeur / récepteur / transmetteur)

Objet

La présente lettre vise à expliquer les détails des modifications apportées aux compteurs dont le type a déjà été approuvé par Mesures Canada. Ces modifications ont été évaluées par le Laboratoire des services d'approbation en conformité aux exigences nationales et doivent être considérées comme faisant partie de la portée des avis d'approbation d'origine énumérés dans le présent document et de toutes leurs révisions subséquentes.

Portée

Les modifications décrites dans la présente lettre s'appliquent aux compteurs visés par les avis d'approbation suivants :

Numéro d'approbation

AG-0546

Requérant

Itron Canada Inc.
6507C Mississauga Road
Mississauga, Ontario
Canada, L5N 1A6

Description des modifications

L'encodeur / récepteur / transmetteur de Itron approuvé sous l'approbation AG-0546 peut être utilisé avec les modèles de compteur principal suivant:

| Fabricant de l'appareil | Modèle | Itron Numéro de pièce |
|--|--|--------------------------------|
| Actaris / Schlumberger | 675A, M675A, 800A, M800A, 1000A, M1000A | ERG-5000-007 |
| Elster American Meter / American Meter Company | 35B, 80B, 250B, 500B, AL800, ALM800, AL1000, ALM1000 | ERG-5000-007 |
| Elster American Meter / American Meter Company | AL1400, AL2300 | ERG-5003-007 and ERG-5003-007P |
| Sensus Metering Systems | RCM-750 | ERG-5003-008 and ERG-5003-008P |

Les compteurs d'Actaris requèrent l'adaptateur # 80005901 celui-ci est disponible chez Actaris.

Copie authentique signée par:

Randy Byrtus, CET
Gestionnaire, Mesure des gaz



Fig. 1: 100G ERT, Part No. ERG-5000-007 (Front View) / N° de pièce ERG-5000-007 (vue de face)

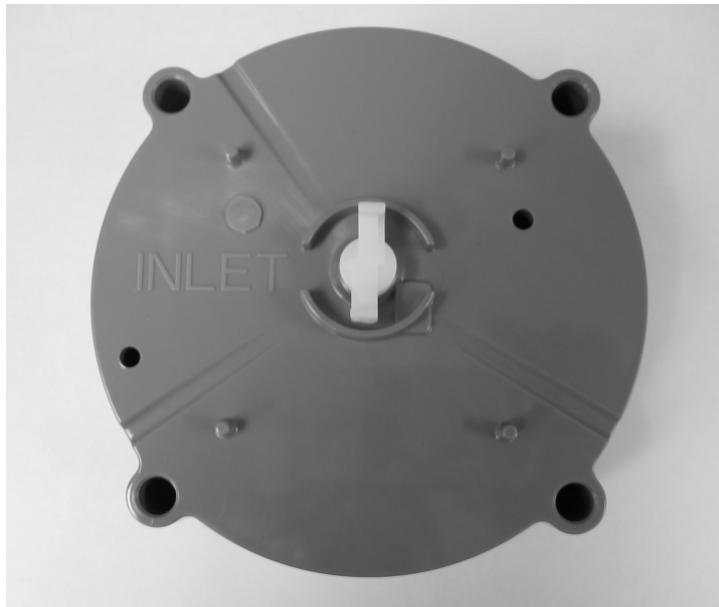


Fig. 2: 100G ERT, Part No. ERG-5000-007 (Rear View) / N° de pièce ERG-5000-007 (vue arrière)