



Consumer and
Corporate Affairs Canada

Consommation
et Corporations Canada

Legal Metrology

Métrologie légale

APPROVAL No. - N° D'APPROBATION
S.WA-T290

MAY 11 1984

NOTICE OF TEMPORARY APPROVAL

Company: Prairie Systems & Equipment
Limited
324 B, 105th Street, East
Saskatoon, Sask.
S7N 1Z3

Manufacturer: Prairie Systems and
Equipment Limited
Saskatoon, Sask.

Type of Device: Electronic hopper scale
that when interfaced to an approved and
compatible digital weight indicator
becomes a weighing system for free
flowing granular materials.

Model Number: PS-GH2-7.5

Maximum capacity: 15 000 lb x 5 lb or
metric equivalent.

- Accessories: Compatible accessories that
meet the requirements and perform in
accordance with the Weights and Measures
Act, Regulations and Specifications may
be used.

Description: This device is an
electronic hopper scale suspended from
two load cells. The load cells are
bolted to two brackets that are fastened
to two "A" frames. Cross braces retain
the "A" frames in position.

The horizontal movement of the hopper is
restricted by chains.

AVIS D'APPROBATION TEMPORAIRE

Société: Prairie Systems & Equipment
Limited
324 B, 105th Street, East
Saskatoon, Sask.
S7N 1Z3

Fabricant: Prairie Systems and
Equipment Limited
Saskatoon, Sask.

Appareil: Trémie de pesage
électronique qui, une fois reliée à un
indicateur pondéral numérique, approuvé
et compatible, forme un ensemble de
pesage pour substances granuleuses à
écoulement libre.

N° de modèle: PS-GH2-7.5


Capacité maximale: 15 000 lb x 5 lb ou
l'équivalent métrique.

Accessoires: Peuvent être utilisés les
accessoires compatibles qui satisfont
aux exigences de la Loi, du Règlement et
des prescriptions ministérielles
régissant les poids et mesures.

Description: Il s'agit d'une trémie de
pesage électronique suspendue à deux
cellules de pesage. Ces cellules de
pesage sont boulonnées à deux supports
fixés à deux chevalets. Les chevalets
sont maintenus en place par des
entretoises.

Des chaînes limitent le déplacement
horizontal de la trémie.

.../2

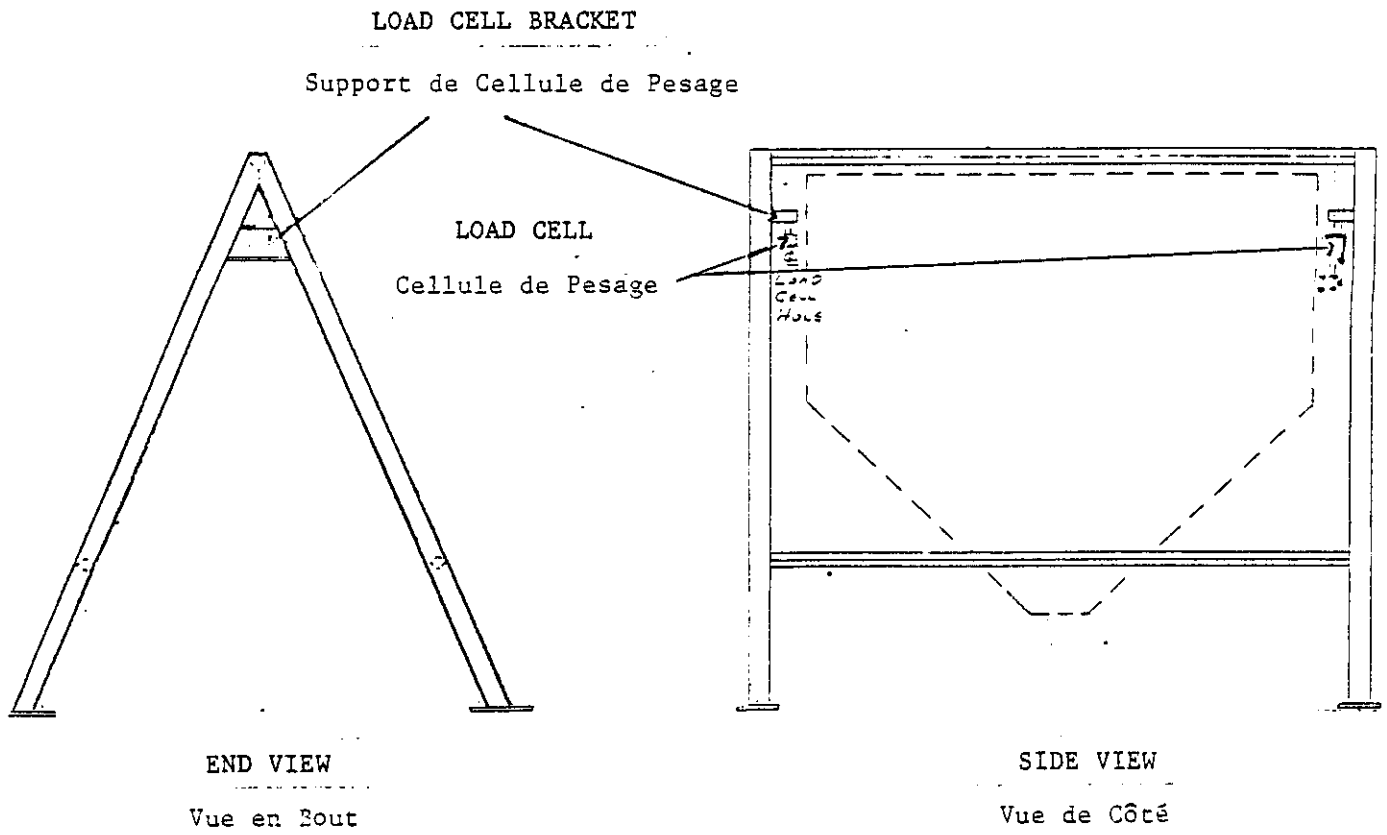

Conditions of Approval:

(1) This approval covers 10 devices only. Each device sold, leased or otherwise disposed of, must be reported to the Head, Mass Laboratory, Legal Metrology Branch in Ottawa, by the manufacturer or distributor.

(2) No device shall be sold, leased or otherwise disposed of, for use in trade, without written disclosure to the purchaser, prior to the sale, that the device has received only temporary approval.

(3) This approval to expire two years from date of issue.

(4) On expiry of this approval only models listed or described having the same nominal capacities and the same nominal physical dimensions and construction as an installation that has been inspected and verified by Weights and Measures, will be considered for full formal approval. After the date of expiry of this Temporary Approval if a model that has not been approved is to be installed, a new application must be submitted, with installation drawings, in order that the Temporary Approval may be reactivated and an inspection arranged.

Reference No.: G6922-P988

Conditions d'approbation:

(1) La présente approbation ne couvre que 10 appareils. Le fabricant ou le distributeur doit faire part de tout appareil vendu, loué ou cédé de quelque autre façon, au Chef du laboratoire des masses, de la Direction de la Métrologie légale, à Ottawa.

(2) Aucun appareil ne doit être vendu, loué ou aliéné de toute autre façon à des fins commerciales sans que l'acheteur n'ait d'abord été avisé par écrit que l'appareil n'a reçu qu'une approbation provisoire.

(3) Le présent avis expire deux ans après sa date d'émission.

(4) Dès expiration du présent avis, seuls les modèles dont les capacités et dimensions nominales ainsi que la construction sont identiques à celles d'une installation déjà inspectée et vérifiée par la Division des poids et mesures seront considérés pour approbation officielle entière. Après la date d'expiration de l'approbation provisoire, pour qu'un modèle non approuvé soit installé, une nouvelle demande devra être présentée avec les plans de l'installation afin que l'approbation provisoire puisse être de nouveau en vigueur et qu'une date d'inspection puisse être fixée.

N° de référence: G6922-P988



W.R. Virtue

Chief
Legal Metrology Laboratories

Chief
Laboratoires de la Métrologie légale

MAY
MAI 11 1984