



Department of consumer and corporate affairs / Ministère de la consommation et des corporations



STANDARDS BRANCH - DIRECTION DES NORMES

NOTICE OF APPROVAL

E-79-1

OTTAWA April 18, 1973.

Canadian General Electric Type "M-30" Demand Register

Types VM-63A and VM-63S transformer type 2-element polyphase watt-hour meters may be fitted with either of the following M-30 Demand Registers:-

One has a register ratio of $333 \frac{1}{3}$, a demand scale of 1.0 kw and a multiplier of 2 and the other has a register ratio of $166 \frac{2}{3}$, a demand scale of 1.5 kw and a multiplier of 1.

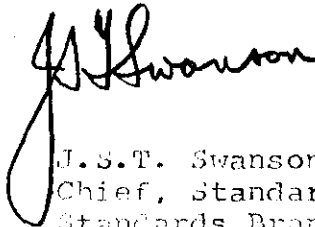
To emphasize the difference in the multipliers, those V-63 meters fitted with demand registers having a register ratio of $166 \frac{2}{3}$ and a demand scale of 1.5 kw should be designated as Type VM-63A2 or VM-63S2 as the case may be.


All other information covered by E-70 remains in full force and effect.

see also circular letter of April 13, 1973.

Approval granted to:

Canadian General Electric Co. Ltd.,
1130 Boulevard Charest
Quebec 8, P.Q.


J.S.T. Swanson, P. Eng.,
Chief, Standards Laboratory,
Standards Branch


W.J.S. Fraser
Chief, Electricity and Gas Division,
Standards Branch

Ref: G 1145-57/C2-125
CL 1145-57/C2-125