



CANADA

SD-WA. 274

DEPARTMENT OF TRADE AND COMMERCE
STANDARDS DIVISION

OTTAWA.....July 25th, 1956.....

APPROVAL LISTING

Equal Arm Dairy Balance - Manufactured by
The Torsion Balance Co., Clifton, New Jersey, U.S.A.

Under the provisions of the Weights and Measures Act, Chapter 292, R.S.C. 1952, and Regulations thereunder (P.C. 6894), the apparatus specified and illustrated herein have been listed as approved devices and may be used in Canada in accordance with the conditions applicable.

Apparatus Listed: Equal arm scales, models DB-1, DB-2, DB-3, and DB-4 with capacities of 240 grams, 240 grams, 240 grams, and 300 grams respectively.

Application: For determining the butter fat content in dairy products.

Conditions: As prescribed in P.C. 6894.


Description: The general design of these devices is similar to DB-5 circular SD-WA. 5, except that the devices are not equipped with a beam, are provided with bottle holding racks and balance is obtained by sliding or turning the rod with knurled knob which protrudes from the side of the scale casing.

Testing: The standard tests for an equal arm scale of similar capacity shall apply and the scale shall be sensitive to .02 grams.

C. S. Phillips,
Assistant Director (W&M),
Standards Division.

R. W. MacLean,
Director,
Standards Division.

Reference: A-399

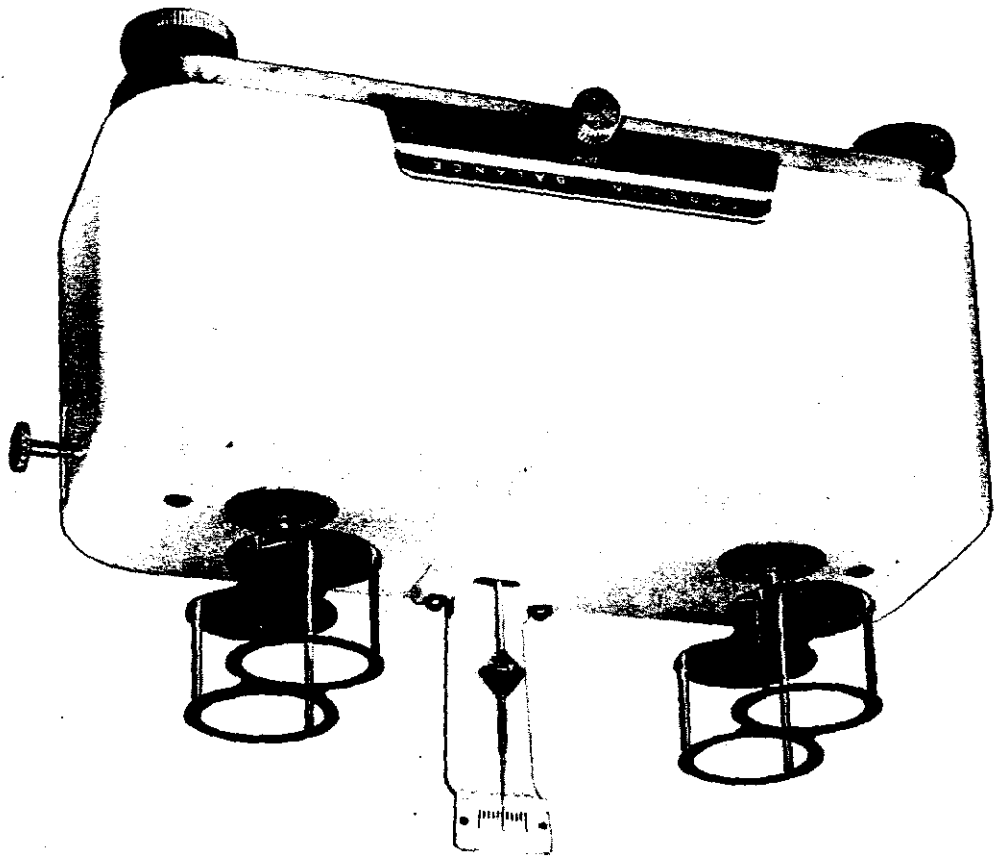

TOBSON DAIRY BALANCE
Model 1B-3

SD-WA.274

